



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Jabe-Alpaca/Jacqueline Tüscher  
Irchelstrasse 26a  
8428 Teufen Switzerland

**Date:** 03/31/17

**Test No:** 940174


### Animal and Sample Description

**Animal Name:** Popham Harlequin  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** White/Dark Fawn

**Animal ID:** 982000148358231  
**Sample Location:** Side  
**Sample Date:** 03/05/17  
**Age:** 07/05/13

### Laboratory Data

<b>Mean Fiber Diameter:</b>	23.2 microns	<b>Fibers Greater Than 30 microns:</b>	10.8 %
<b>Standard Deviation:</b>	5.8 microns	<b>Comfort Factor:</b>	89.2 %
<b>Coefficient of Variation:</b>	24.8 %	<b>Mean Curvature:</b>	42.9 deg/mm
<b>Spin Fineness:</b>	23.4 microns	<b>SD Curvature:</b>	35.7 deg/mm

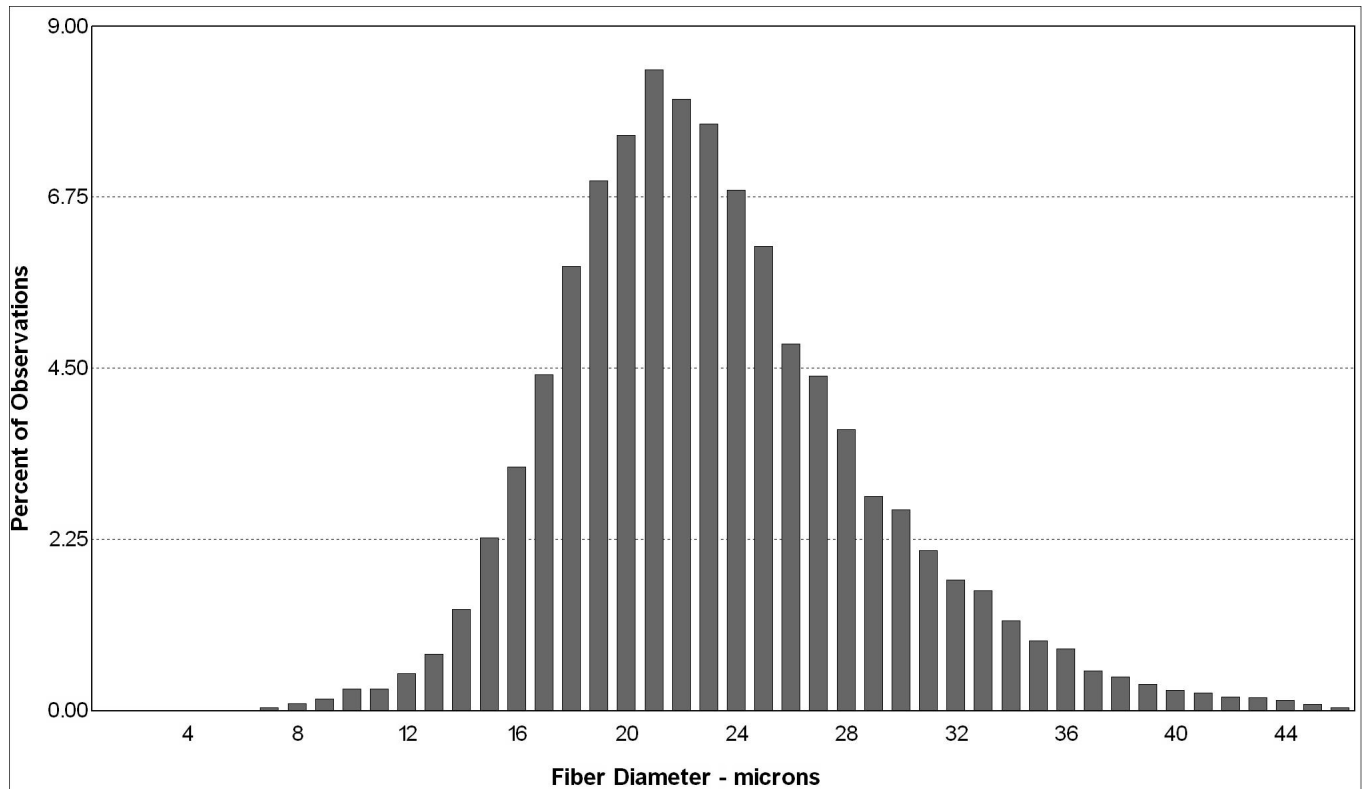

This Test Performed According to I.W.T.O Method 47