



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

NWKS Neuweltkameliden Schweiz/Sven Baumgartner  
Rheinhofstrasse 11  
Salez 9465 CH

07/02/13

Test No: 457178


### Animal and Sample Description

**Animal Name:** BBA Farah (Glaus-Risi)  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** BG

**Animal ID:** 35703  
**Sample Location:** Side  
**Sample Date:** 03/29/13  
**Age:** 09/09/08

### Laboratory Data

<b>Mean Fiber Diameter:</b>	23.9 microns	<b>Spin Fineness:</b>	23.4 microns
<b>Standard Deviation:</b>	5.2 microns	<b>Mean Curvature (deg/mm):</b>	39.4
<b>Coefficient of Variation:</b>	21.6 %	<b>SD Curvature (deg/mm):</b>	24.8
<b>Fibers Greater Than 30 microns:</b>	11.1 %	<b>Comfort Factor:</b>	88.9 %

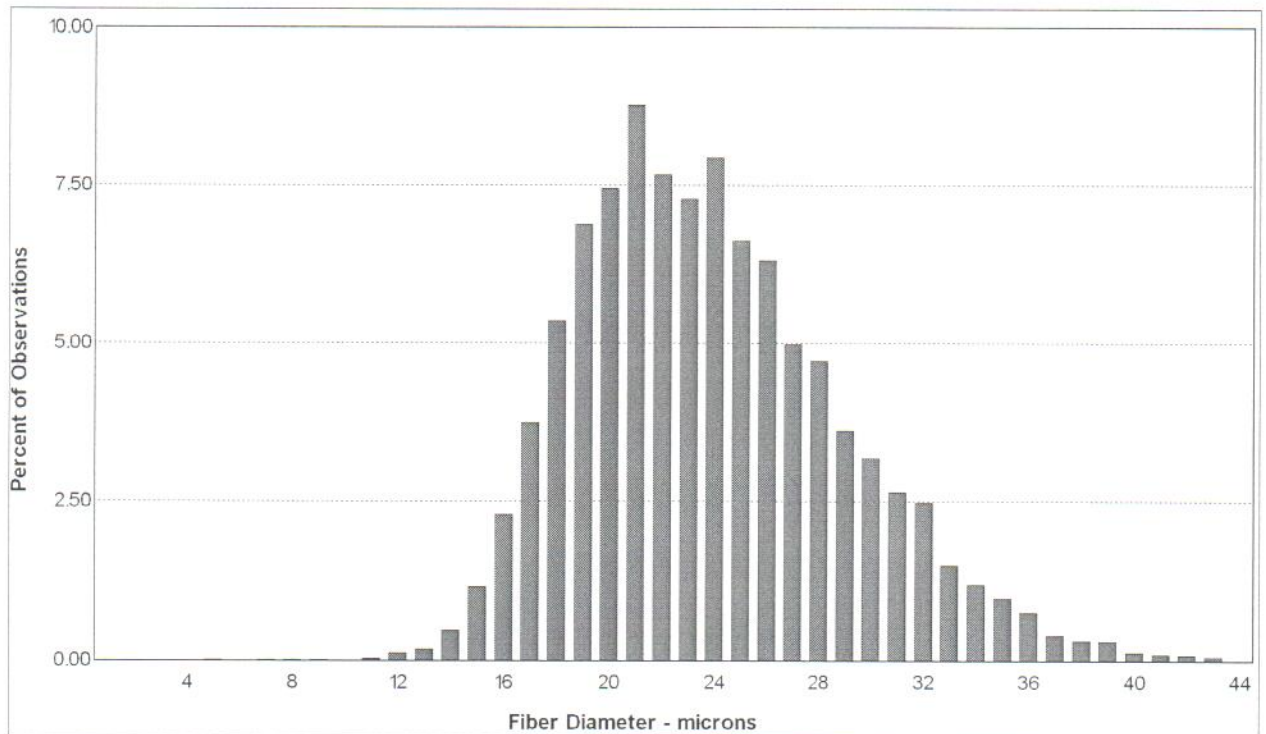

This Test Performed According to I.W.T.O Method 47