



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Jabe Alpaca/Jacqueline Tüscher
Am Burghügel 9
8427 Freienstein 8427 Switzerland

Date: 09/24/15

Test No: 914601


Animal and Sample Description

Animal Name: Marie-Louise
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 982000362837567
Sample Location: Side
Sample Date: 05/15/15
Age: 06/28/13

Laboratory Data

Mean Fiber Diameter:	16.5 microns	Fibers Greater Than 30 microns:	1.0 %
Standard Deviation:	4.0 microns	Comfort Factor:	99.0 %
Coefficient of Variation:	24.4 %	Mean Curvature:	50.3 deg/mm
Spin Fineness:	16.5 microns	SD Curvature:	27.0 deg/mm

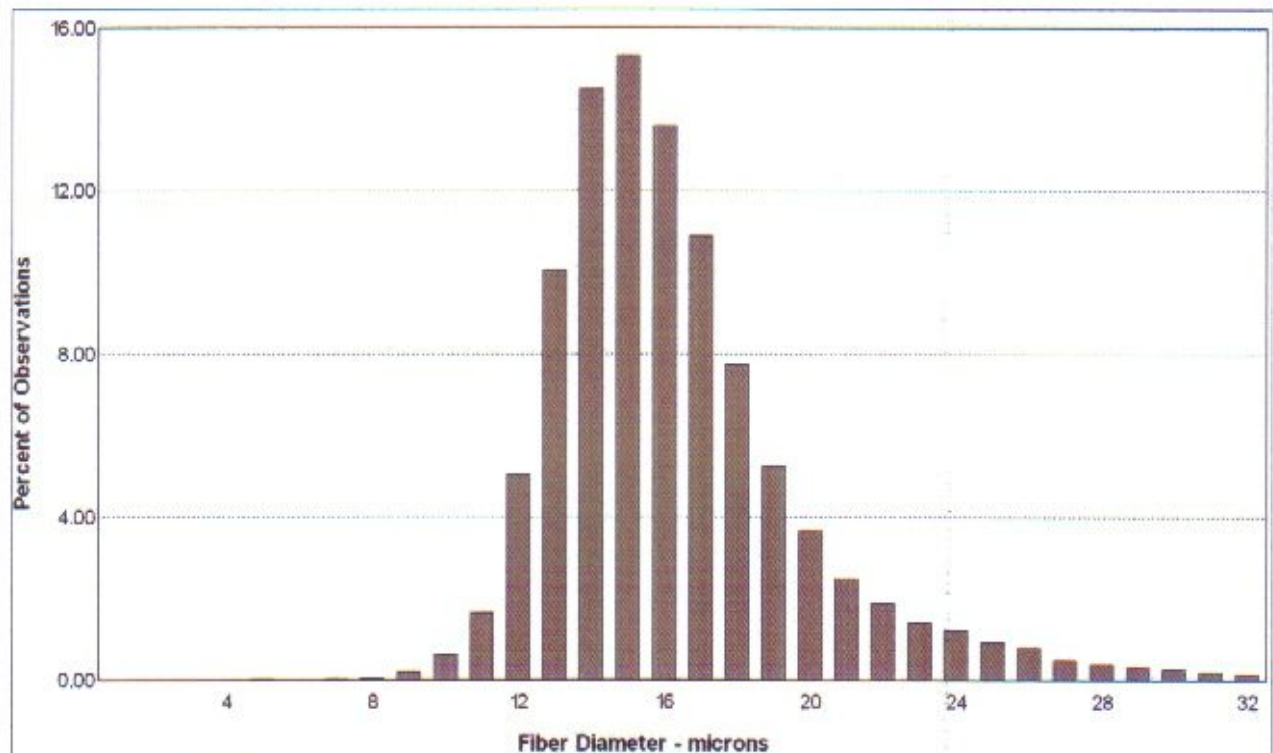

This Test Performed According to I.W.T.O Method 47