



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Jabe Alpaca/Jacqueline Tüscher  
Am Burghügel 9  
8427 Freienstein 8427 Switzerland

**Date:** 09/24/15

**Test No:** 914600


### Animal and Sample Description

**Animal Name:** Popham Appaloosa Harlequin  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** White/Dark Fawn

**Animal ID:** 982000148358231  
**Sample Location:** Side  
**Sample Date:** 04/15/15  
**Age:** 05/04/13

### Laboratory Data

<b>Mean Fiber Diameter:</b>	20.7 microns	<b>Fibers Greater Than 30 microns:</b>	4.7 %
<b>Standard Deviation:</b>	5.1 microns	<b>Comfort Factor:</b>	95.3 %
<b>Coefficient of Variation:</b>	24.5 %	<b>Mean Curvature:</b>	40.7 deg/mm
<b>Spin Fineness:</b>	20.8 microns	<b>SD Curvature:</b>	25.0 deg/mm

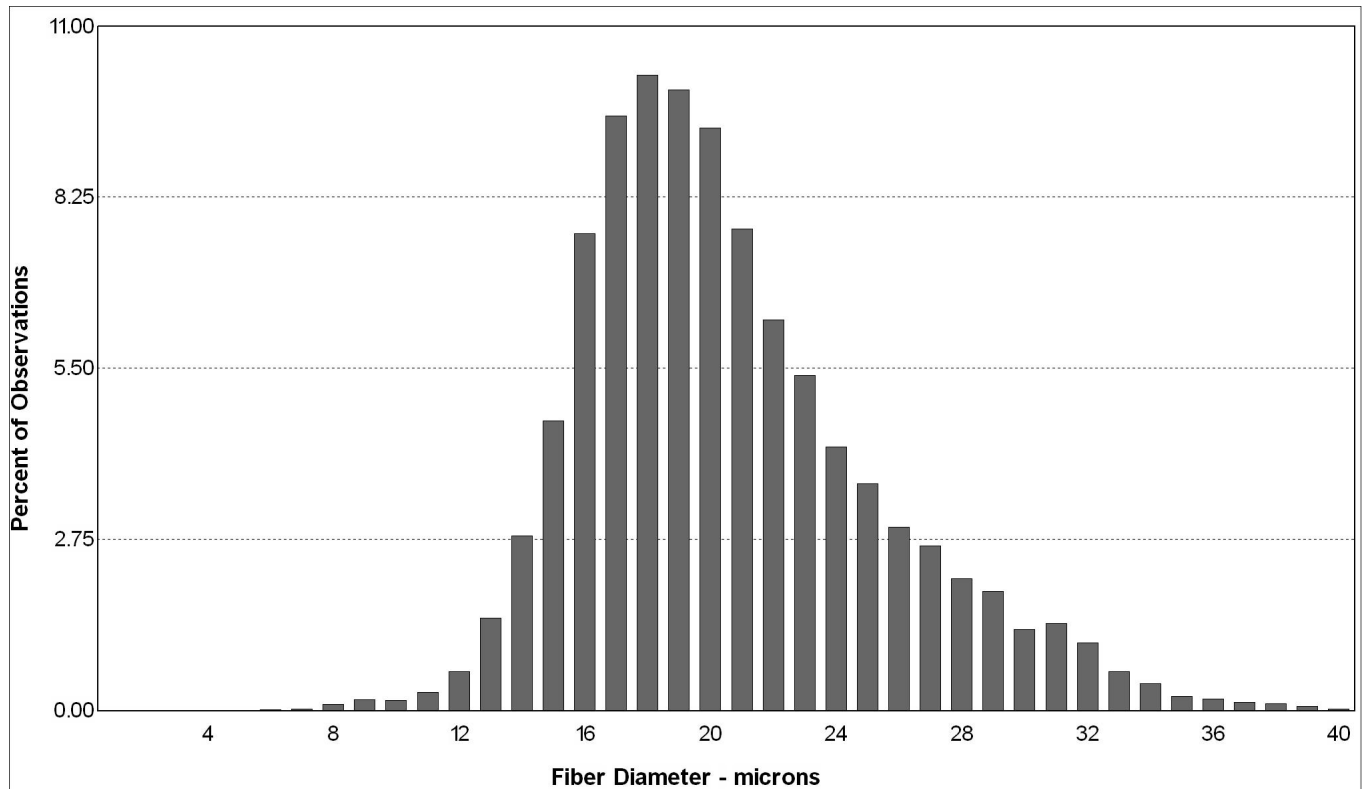

This Test Performed According to I.W.T.O Method 47