

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

NWKS Neuweltkameliden Schweiz/Sven Baumgartner  
Rheinhofstrasse 11  
9465 Salez, Switzerland

Date: 01/29/14

Test No: 473510


### Animal and Sample Description

**Animal Name:** Fujiyama (Kyburz)  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** 100 W

**Animal ID:** 39233  
**Sample Location:** Side  
**Sample Date:** 11/14/13  
**Age:** 06/11/09

### Laboratory Data

<b>Mean Fiber Diameter:</b>	21.4 microns	<b>Fibers Greater Than 30 microns:</b>	3.2 %
<b>Standard Deviation:</b>	4.7 microns	<b>Comfort Factor:</b>	96.8 %
<b>Coefficient of Variation:</b>	21.8 %	<b>Mean Curvature:</b>	51.5 deg/mm
<b>Spin Fineness:</b>	21.0 microns	<b>SD Curvature:</b>	27.1 deg/mm

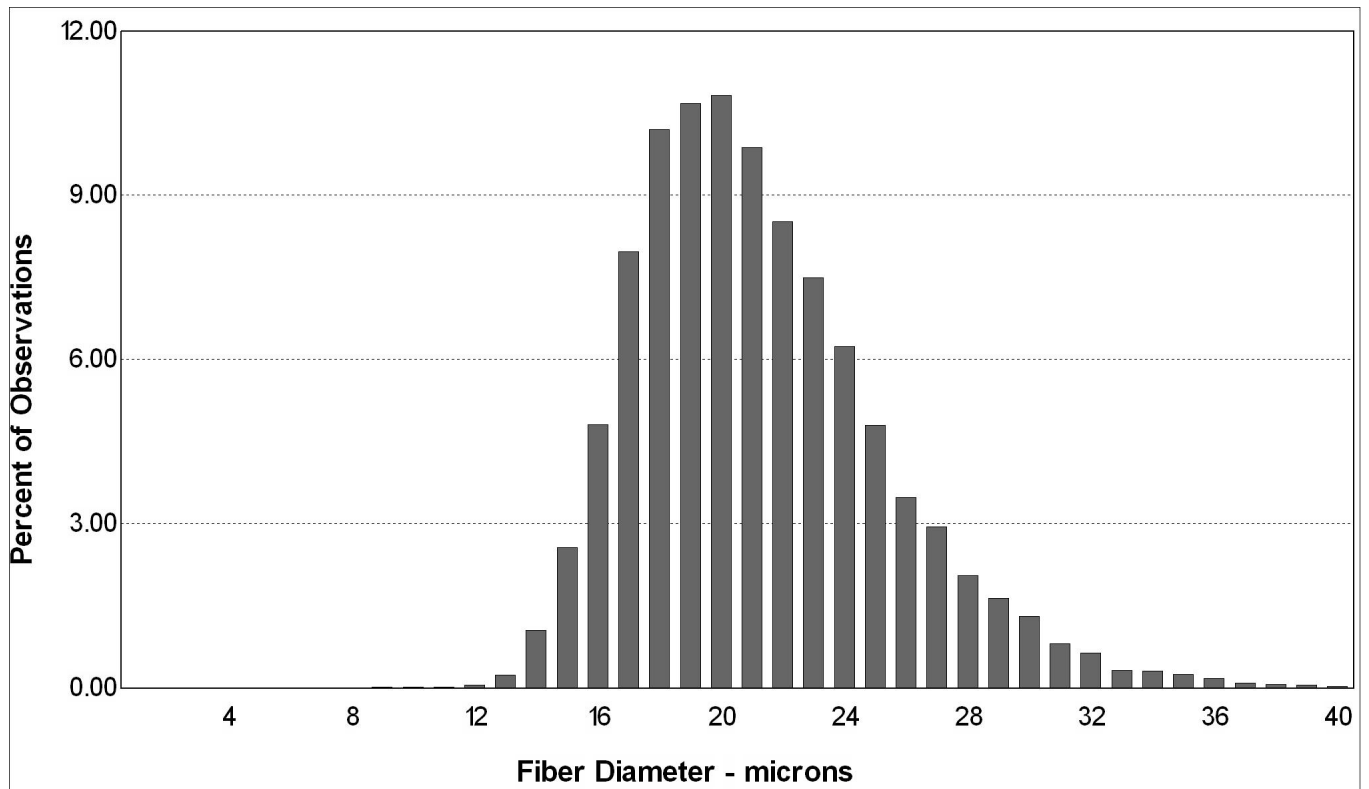

This Test Performed According to I.W.T.O Method 47